

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAY 20 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130181</u>	
Name <u>Michael A. Wery</u>		ID# <u>3590</u>	Date <u>4-23-10</u>
A	Agency <u>AST</u>	Phone # <u>451-2850</u>	
Instrument Location <u>Nenana AST</u>			
Alco S/N <u>78895</u>		Target Value <u>.074</u>	High Pressure <u>850</u>
B	Alco Test Value Average <u>.077</u>		
	1 st Alco	<u>.077</u>	2 nd Alco
Signature <u>[Signature]</u>		<u>CB</u> <u>5/24/10</u>	
(OVER)			

(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 18th day of June, 2010.

[Signature]
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

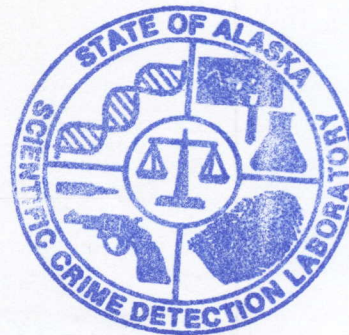

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130181 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130181 ✓

APRIL 23, 2010 ✓ *CUS 5/24/10*

OPERATOR'S NAME:
WEYER-MICHAEL/A
OPERATOR'S NUMBER: 3590
SUBJECT'S LAST NAME:
VERIFICATION
SUBJECT'S FIRST NAME/MI :
OF CALIBRATION
O.L. #: 8
DEPT/AGENCY: MEMO
CASE/REPORT:
TEST TYPE: V
ALCO TARGET VALUE: .074 ✓
ALCO S/N: 78895 ✓

— BREATH ANALYSIS —

.074 ADJUSTED FOR 29.77 in ✓

ALCO TARGET	.073	17:30
BLANK TEST	.000	17:31
INTERNAL STANDARD	VERIFIED	17:31
ALCO TV 29.77 in	.077 ✓	17:31
BLANK TEST	.000	17:32
SUBJECT SAMPLE <i>CUS 5/24/10</i>	.000 ✓	17:33
BLANK TEST	.000 ✓	17:34
ALCO TV 29.77 in	.077	17:34
BLANK TEST	.000	17:35

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130181 ✓

APRIL 23, 2010 ✓
TIME 17:27

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/28/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 29.77 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~